

# DeltaVen® Technical Data Sheet

## Single Port with Stopcock and Needleless Connector

### DEVICE CLASSIFICATION

Class IIa

### DEVICE DESCRIPTION

Closed system safety I.V. Catheter in polyurethane (PUR) with accessories.

### GMDN

40601

### CE MARK

CE 0123


### COUNTRY OF ORIGIN

Italy

### ANIMAL ORIGIN

The devices listed on this product family are free from animal origin or have undergone inactivation of TSE/BSE agent's process.

### DIAGRAM

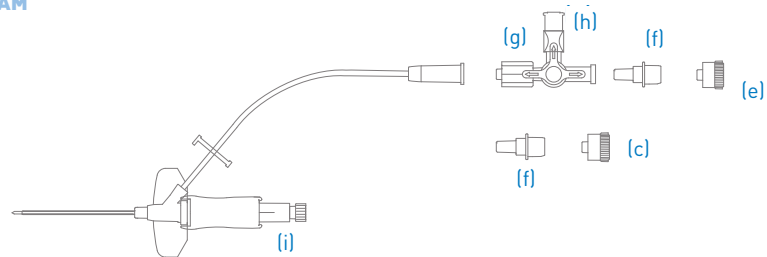

### STERILIZATION METHOD

Ethylene Oxide

### MANUFACTURING SITE NAME AND ADDRESS

Delta Med SpA  
Via G. Rossa, 20-46019  
Viadana (Mn) – Italy  
0375 785915

### PRODUCT DESCRIPTION

DeltaVen® is a radio-opaque polyurethane catheter equipped with a rubber septum inside which a stainless steel needle is inserted. The catheter is connected to a lateral extension whose end section is connected to a single port Luer-lock fitting (i) connected to a three way-stopcock (g) and integrated needleless connector (h). The end section of the stopcock is connected to an air vent plug (f), on which a Luer-lock cap (e) is assembled. The catheter is also equipped with a passive safety system designed to prevent needlestick injuries.

### PRECAUTIONS

Use of the device is for medical or paramedical competence.

- Read the instructions before use.
- Use protective gloves.
- Do not use if the individual packaging is damaged or open or if the product is past the "use by" date.
- Do not use if the device is incomplete or has been tampered with.
- The product must be used immediately after the packaging has been opened.
- Do not attempt to reinsert the entry needle in the rubber septum it was extracted from.
- Do not reinsert the needle while the catheter is located wholly or partly on site. It could break the catheter.
- Do not insert needles, sharp objects or faulty connectors in the needleless connector. It could cause leakages from the device. In case of an attempted insertion of a needle or a blunt cannula, replace the needleless connector.
- Replace stopcock within a maximum time of 3 days or 24 hours if concentrated glucose, lipidic or blood-derived solutions are being used. Needleless connector must be replaced after 200 activations.
- Do not use needleless connector access with an operating pressure exceeding 2 bar.

- Disposable device: Do not sterilise and/or reuse in order to avoid compromising functionality or aid possible cross contamination with other patients.
- After use, dispose of as hospital waste.
- In case of incorrect transport and/or manipulation, the device or packaging could be subject to structural and/or functional damage.
- Do not use scissors at or near the insertion site.
- Do not remove the security system from the catheter prior to use.
- Use only Luer-lock connectors and caps (ISO 594-2).

#### If the device is used at a high pressure or with injectors:

- Connect directly to the pressure infusion system with the end Luer-lock connector of the device.
- Remove the stopcock connected to the device.
- Always check the patency of the device before use.
- Never exceed the maximum pressure of 23 bar (330 psi).

- Consider the internal residual volume of the device in the case of administration of small volumes of medicines.
- If pain, swelling around the catheter insertion area or the occurrence of edema/erythema or other local complications are experienced, replace the device and insert a new one in another site.
- Clean the device immediately after the administration of medicines or biological fluids.
- Immediately remove any needle that has no coating, always keeping the tip away from your body and fingers.
- Do not expose to heat or direct sunlight.
- If the catheter is incorrectly inserted under the skin, remove it and never try to re-insert the needle into the catheter when it was extracted partially or totally.
- If during insertion under the skin blood appears in the needle mounting unit or in the catheter after withdrawing the needle, discard the device and insert in another place.
- If you want to administer a drug bolus different from what is being administered subcutaneously in a continuous mode, you must insert a new catheter to avoid incompatibilities between drugs.

## INDICATIONS

DeltaVen® is a catheter for peripheral venous and subcutaneous access that, in combination with other peripheral devices, allows the collection of blood samples and the administration of fluids. DeltaVen® is intended to be used for less than 30 days.

DeltaVen® is equipped with a passive system for the prevention of accidental needlestick injuries. During the initial insertion phase, the blood remains in the device facilitating the prevention of exposure to blood. Take into account the vascular anatomy of the patient and of the adequacy of the procedure.

DeltaVen® catheters are suitable for use with pressure injectors (max. 330 psi) only if all accessories are removed. The recommended measurements for subcutaneous use are 26G, 24G and 22G with a 19 mm catheter length. DeltaVen® 26G: DO NOT USE FOR HIGH PRESSURE TREATMENTS.

## PRODUCT COMPONENTS

Non-pyrogenic, sterile, single-use device. The device is not made of natural latex and phthalates.

DeltaVen® is a radio-opaque polyurethane catheter equipped with a rubber septum inside which a stainless steel needle is inserted. The catheter is connected to a lateral extension line (i) whose end section is connected to a three way stopcock (g) with a needleless connector integrated (h). The end section of the stopcock is connected to an air vent plug (f), on which a Luer-lock cap (e) is assembled. The catheter is also equipped with a passive safety system designed to prevent needlestick injuries.

## COMPONENT COMPOSITION

Polyurethane catheter with three radio-opaque strips enclosed in the wall containing BaSO<sub>4</sub>.

- AISI304 stainless steel needle.
- Polycarbonate catheter hub.
- Silicone rubber septum needle seal.
- Butterfly with polypropylene body and thermoplastic synthetic rubber wings.
- Polyurethane extension line DEHP free.
- ABS colored Luer-lock connection.
- Styrene butadiene copolymer air vent with high density polyethylene hydrophobic filter.
- Polypropylene Luer-lock cap.
- Polycarbonate stopcock with silicone rubber needleless connector.

## LABELLING AND PACKAGING

Container Type	Length	Width	Height	Weight
Unit Pack (1 unit)	140 mm	60 mm	25 mm	0.011 kg
Shelf Pack (20 units)	295 mm	140 mm	95 mm	0.35 kg
Case Pack (80units)	395 mm	305 mm	160 mm	1.7 kg

PRODUCT(S) DESCRIBED MAY NOT BE LICENSED OR AVAILABLE FOR SALE IN CANADA AND OTHER COUNTRIES

**Distributed by:**  
**Smiths Medical International**  
1500 Eureka Park, Lower Pemberton  
Ashford Kent, TN25 4BF  
Tel: +44 (0)845 850 0445

**Manufactured by:**  
**Delta Med SpA**  
Via G. Rossa, 20-46019  
Viadana (Mn) – Italy  
0375 785915

**MPAUCA-1737**

Find your local contact information at: [www.smiths-medical.com/customer-support](http://www.smiths-medical.com/customer-support)

**smiths medical**

Smiths Medical is part of the global technology business Smiths Group plc. Please see the Instructions for Use/Operator's Manual for a complete listing of the indications, contraindications, warnings and precautions. The Smiths Medical design mark is a trademark of Smiths Medical. The symbol ® indicates the trademark is registered in the U.S. Patent and Trademark Office and certain other countries. All other names and marks mentioned are the trademarks or service marks of their respective owners. The product referenced is CE-marked. ©2017 Smiths Medical. All rights reserved. SS195481GB-092017